


Overview EQA II/2024

Sample 2024-05: CT negative / NG positive

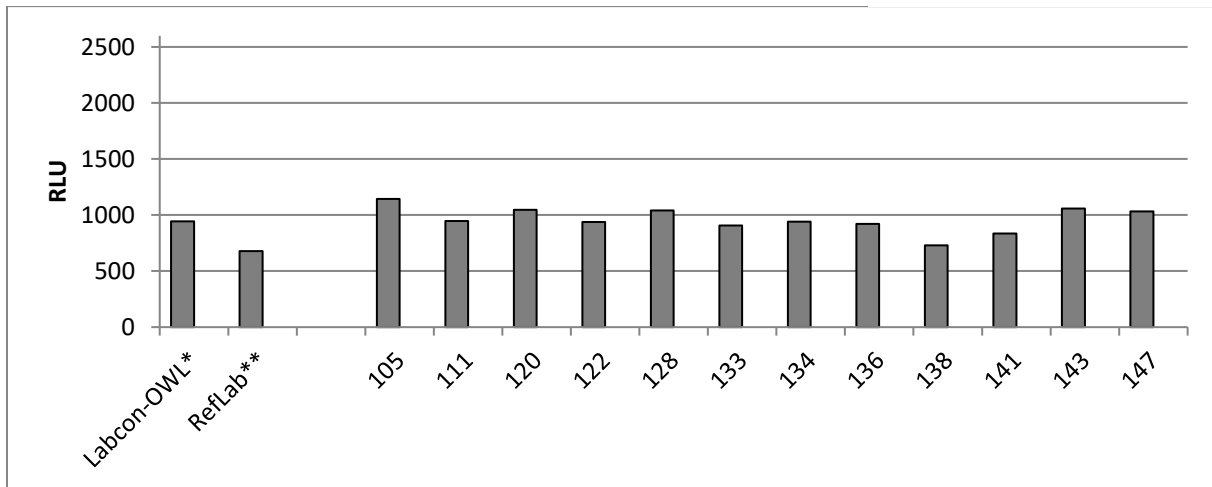


	RLU Panther
LABCON-OWL*	943
RefLab**	678
105	1145
111	948
120	1047
122	939
128	1040
133	907
134	942
136	920
138	729
141	836
143	1058
147	1034

*RLU value constantly monitored over the entire testing phase of the external quality assessment by LABCON-OWL GmbH

**External Reference Laboratory in Germany

Sample 2024-06: CT positive / NG positive

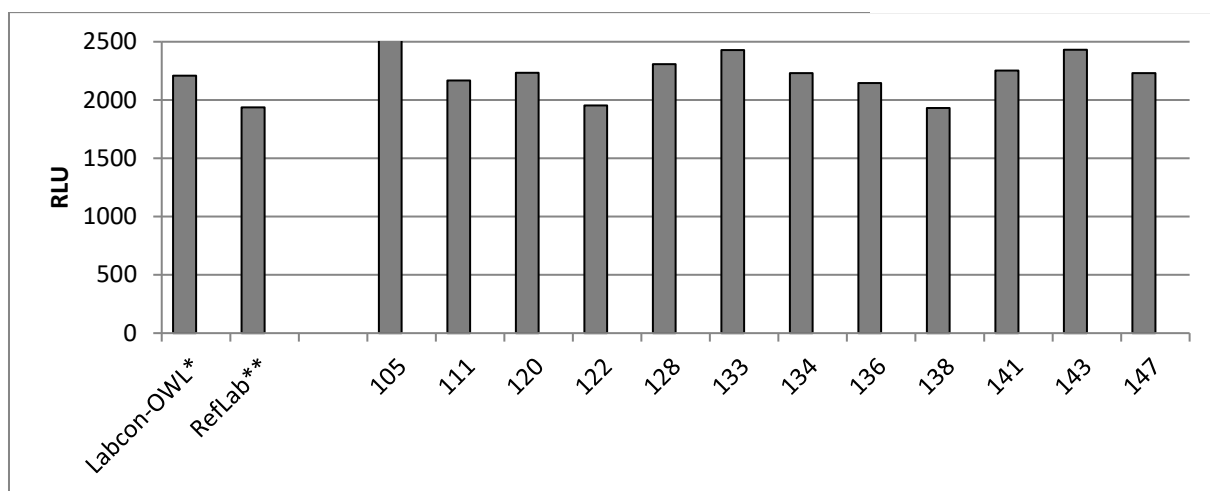


	RLU Panther
LABCON-OWL*	2209
RefLab**	1936
105	2520
111	2169
120	2233
122	1954
128	2308
133	2429
134	2232
136	2145
138	1932
141	2252
143	2431
147	2231

*RLU value constantly monitored over the entire testing phase of the external quality assessment by LABCON-OWL

**External Reference Laboratory in Germany

Sample 2024-07: CT positive / NG negative

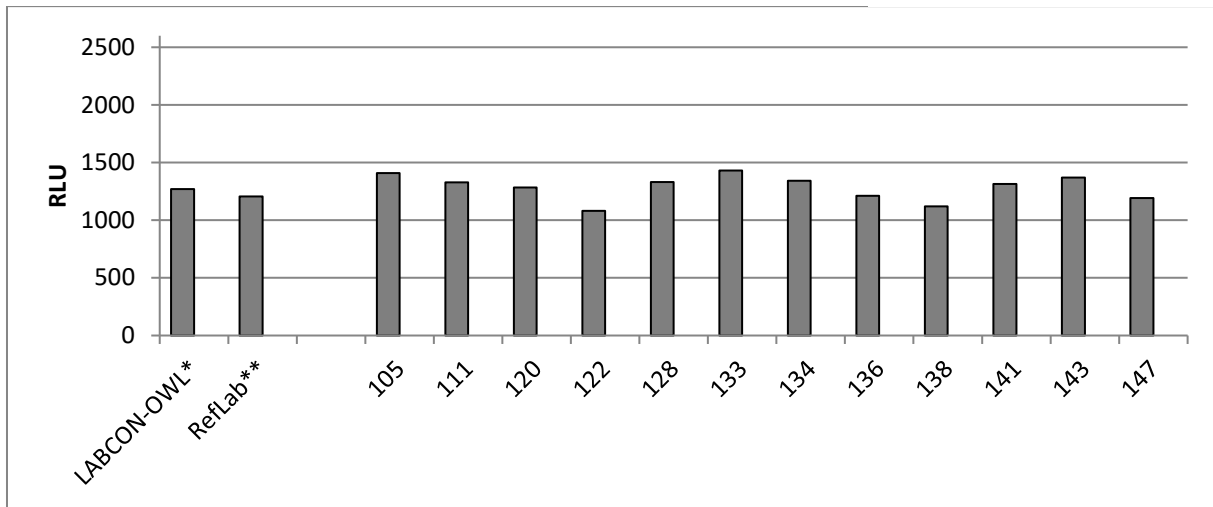


	RLU Panther
LABCON-OWL*	1270
RefLab**	1205
105	1410
111	1328
120	1285
122	1081
128	1332
133	1430
134	1342
136	1211
138	1121
141	1314
143	1369
147	1193

*RLU value constantly monitored over the entire testing phase of the external quality assessment by LABCON-OWL

**External Reference Laboratory in Germany

Sample 2024-08: CT negative / NG negative

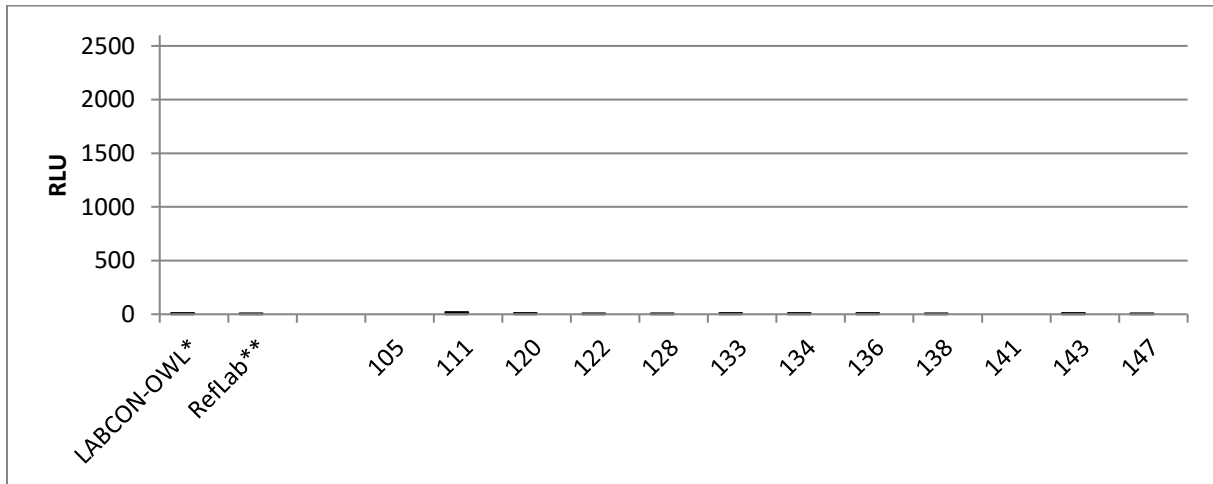


	RLU Panther
LABCON-OWL*	10
RefLab**	7
105	-
111	20
120	10
122	7
128	9
133	11
134	11
136	10
138	9
141	-
143	11
147	7

*RLU value constantly monitored over the entire testing phase of the external quality assessment by LABCON-OWL

**External Reference Laboratory in Germany

Appendix: Stability of the samples over the period of the external quality assessment

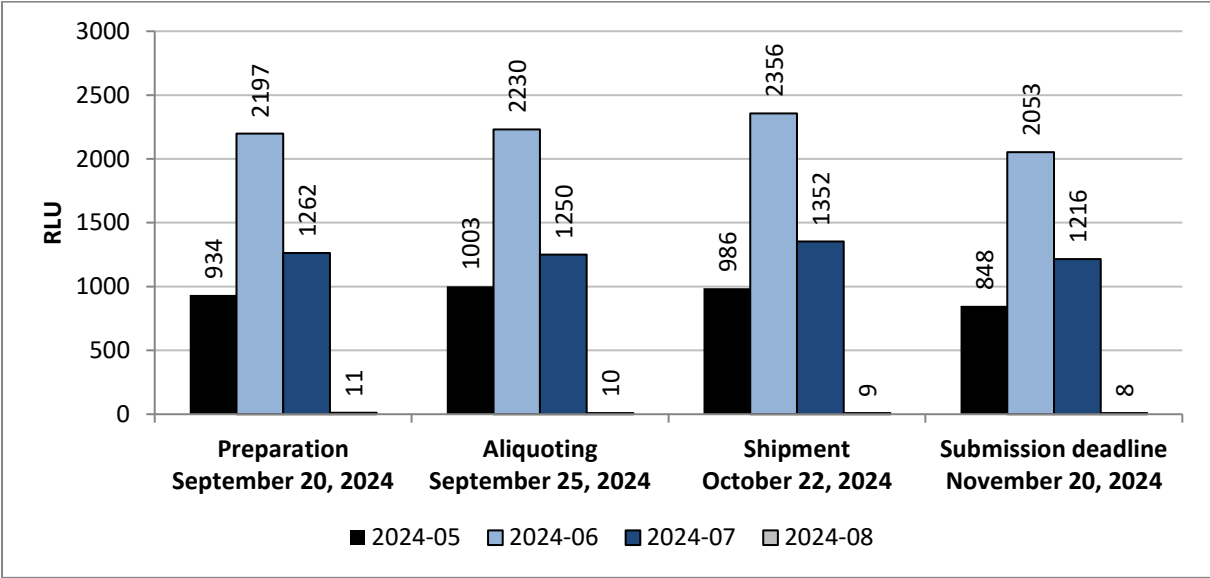

RLU values determined over the period of the external quality assessment by LABCON-OWL

The target value of all samples was confirmed and monitored in a reference laboratory in Germany before distribution. During the testing period the samples were retested three times by LABCON-OWL. The data are illustrated above. This graph shows the course of signal change for all four panel members over a period of ten weeks (storage at room temperature).